

Simultaneous speciation analysis of As, Sb and Se redox couples by SF-ICP-MS coupled to HPLC

Cite this: *Anal. Methods*, 2014, 6, 5112

Debo Wu* and Thomas Pichler

A new method was developed for the simultaneous speciation analysis of inorganic arsenic (iii, v), antimony (iii, v) and selenium (iv, vi) in fluid samples by double-focusing sector field-inductively coupled plasma-mass spectrometry (SF-ICP-MS) coupled with high performance liquid chromatography (HPLC). A Hamilton PRX-X100 anion exchange column with EDTA (pH of 4.7) and 3% methanol as mobile phase was used for separation of the six species. The flow rate was set at 1.5 mL min⁻¹. The overall analysis time was shortened down to within 11 minutes for all six desired species after a solvent gradient (linear ramp from 5 mM to 30 mM) was introduced in. The detection limits for As(III), As(V), Sb(III), Sb(V), Se(VI) and Se(IV) were 0.02 µg L⁻¹, 0.06 µg L⁻¹, 0.2 µg L⁻¹, 0.02 µg L⁻¹, 0.2 µg L⁻¹ and 0.4 µg L⁻¹ respectively, which were obtained from 11 replicate measurements of blank. The stability of retention time and linearity of calibration curve were also evaluated. Relative standard deviations (RSD) of ≤9% for retention times (at least 20 replicate measurements) and correlation coefficients (*R*²) of ≥0.9998 for calibration curves (at least 6 replicate experiments) were obtained. Finally, the proposed method was applied to the analysis of one synthetic sample, two hot spring samples and two certified reference materials. The results showed a good spike recovery, indicating that basically no mass loss occurred during chromatographic separation. For two certified reference materials, the detected results were in good agreement with the certified values.

Received 28th April 2014
Accepted 24th May 2014

DOI: 10.1039/c4ay01013b

www.rsc.org/methods

1. Introduction

Despite our effort to better understand the geochemistry of redox sensitive, multi species elements, such as, arsenic (As), antimony (Sb), chromium (Cr), cobalt (Co), copper (Cu) and selenium (Se), there are still large gaps in our knowledge, particularly with respect to their redox behavior in different environments. It has been realized that a full understanding of the redox behavior of these species can help us to: (a) better understand the redox behavior of these elements in different matrices;¹⁻³ (b) develop further studies in the area of toxicity and bioavailability, for example, different toxicity and bioavailability as a function of redox state;⁴⁻⁷ (c) evaluate competitive adsorption of, for example, arsenic and antimony, onto hydrous ferric oxide (HFO) surfaces, which in turn would let us better predict their mobility.⁸⁻¹⁰ However, conventional total element concentration determination did not provide adequate information to completely understand the effect, behavior and fate of these redox species in the environment. In view of this hyphenated analytical techniques such as HPLC-HG-AFS, ETV-ICP-MS¹¹ and HPLC-ICP-MS¹² were developed to obtain additional information about the distribution of individual redox

species. Since the distribution of redox species of a given element in an aqueous solution greatly depends on the species distribution in other redox couples an accurate and rapid simultaneous speciation analysis method for multiple redox couples would be the logical next step towards an improved understanding of redox chemistry in natural systems.

Redox speciation analysis requires analytical technology, which basically includes species separation followed by detection, where due to often low concentrations and minute sample amounts detector can be the weak link. If it is desired to speciate more than one redox couple chromatographic separation becomes critical and difficult, because the chromatography conditions for different elements can vary substantially. For example, inorganic As species are usually separated with anion exchange chromatography with phosphate buffers at neutral pH as mobile phase^{13,14} and anion exchange column such as Hamilton PRP-X100 column is most commonly used.^{15,16} Se species are commonly separated with anion exchange chromatography as well, with phosphate, ammonium or citrate buffers as mobile phase.¹⁷ However, Sb behaves quite differently, as it has complexing properties and needs the presence of a chelating agent in the mobile phase. EDTA¹⁸⁻²⁰ and phthalic acid²¹⁻²⁴ have been widely used as mobile phase. In the wide pH range from 2 to 10 in aqueous solutions, Sb(III) exists in the form of non-charged Sb(OH)₃⁰ in liquid, while Sb(V) exists as negatively charged Sb(OH)₆⁻.²⁵ Theoretically, Sb(OH)₃⁰ and

Geochemistry & Hydrogeology, Department of Geosciences GEO, Bremen University, 28334 Bremen, PO Box 330440, Germany. E-mail: debo.wu@uni-bremen.de; Fax: +49 (0) 421-218-65105; Tel: +49 (0) 421-218-65119

Sb(OH)_6^- can be separated using an anion exchange column, then Sb(OH)_3° would be eluted in solvent-front, and Sb(OH)_6^- would be retained in the column and eluted out subsequently. However, the fact is that Sb(OH)_6^- elutes close to the solvent front and Sb(OH)_3° is strongly retained in the column and can not be eluted with common mobile phases similar to those used for As and Se speciation. This provides a challenging task in finding the optimum mobile phase, which would allow the separation of As, Se and Sb redox couples. A few methods for the simultaneous speciation analysis of As, Sb and Se are listed in Table 1. Only one of the methods, however, allowed complete speciation analysis of the three redox couples, and was only optimized with synthetic standards.²⁶ Guerin *et al.*¹⁷ developed a speciation analysis method for As(III, V), Se(IV, VI) and Sb(V), but Sb(III) was not included. Iserte *et al.*²⁷ and Morita *et al.*²⁸ only considered the speciation analysis of two of the three elements. Regarding the stationary phases, anion exchange was the typical choice for the simultaneous separation of those species. However, Morita *et al.*²⁸ used a reversed phase chromatographic column, basically because they were interested in the separation of other organic As species. For the separation of As and Se species, phosphate and hydrogen carbonate buffers are adequate, when anion exchange chromatography is used. If Sb should be separated together with Se and As species, a chelating agent, such as tartaric acid, malonic acid or EDTA is usually added.

Following a successful chromatographic separation of the three redox couples, simultaneous detection and thus speciation analysis still requires sensitive detection. ICP-AES, ICP-AAS and AFS were extensively investigated but not practically applied, because of low sensitivity and spectral interferences specially for Se.^{29–32} Thus an extra analytical step, such as hydride generation (HG), was used to improve its sensitivity.^{33–35} However, HG-ICP-AES, HG-ICP-AAS, HG-AFS are not suitable for direct Se(VI) determination, due to its inability to form a Se-hydride.^{30,36–38}

In this paper we presented a new method for the simultaneous speciation analysis of As(III, V), Sb(III, V), and Se(IV, VI) using double-focusing sector field-inductively coupled plasma-mass spectrometry (SF-ICP-MS) coupled to high performance liquid chromatography (HPLC). In addition to low detection limits and good separation one of the goals was to keep the chromatographic conditions as simple as possible, with the idea that this should facilitate implementation of this method by others interested in the redox behavior of natural aqueous solutions.

2. Experimental

2.1 Instrumentation

2.1.1 Detection. A Thermo Scientific ELEMENT 2 sector field ICP-MS (SF-ICP-MS) was used for the detection of As(III, V),

Table 1 Review of various chromatography methods of simultaneous separation of inorganic species of As, Sb and Se^a

	Matrix	Column	Eluent	Species	Method information	Reference
As, Se	Sediment, extracts	Anion exchange Hamilton PRX-X100 (250 mm × 4.1 mm, 10 μm)	Gradient elution: A: 10 mM $\text{NH}_4\text{H}_2\text{PO}_4$ pH = 6 (with ammonia) B: 200 mM $\text{NH}_4\text{H}_2\text{PO}_4$ pH = 6 (with ammonia)	As(III), As(V), MA(V), DMA(V), Se(IV), Se(VI)	Flow = 1.0 mL min ⁻¹ , injection volume = 100 μL, time: <10 min, LOD*: 2–40 ng g ⁻¹ , spike recovery: 80–120%, (except As)	27
As, Se, Sb	Standards	Dionex IonPac AS14, (250 mm × 4 mm) with IonPak AG 14, (50 mm × 4 mm)	Gradient elution: A: 2 mM ammonium hydrogen carbonate + 2.2 mM tartaric acid pH = 8.2 (with ammonia) B: 2 mM ammonium hydrogen carbonate + 45 mM tartaric acid pH = 8.2 (with ammonia)	As(III), As(V), MA(V), DMA(V), Se(IV), Se(VI), Sb(III), Sb(V)	Flow = 1.0 mL min ⁻¹ , injection volume = 50 μL, time: ≈ 15 min, LOD*: 4.5 μg L ⁻¹ (Sb(III) and Se species) 0.5 μg L ⁻¹ (others) RSD [#] (retention time): <2%	26
As, Sb	Hot spring water, fish sample	Develosil C30-UG-5 (250 mm × 4.6 mm, 5 μm)	Isocratic elution: 10 mM sodium butanesulfonate + 4 mM malonic acid + 4 mM tetramethylammonium hydroxide + 0.1% (v/v) methanol 20 mM ammonium tartrate pH = 2.0	As(III), As(V), MA(V), DMA(V), AsB, AsC, TMAO, TeMA, Sb(III), Sb(V)	Flow = 0.75 mL min ⁻¹ , injection volume = 10 μL, time: ≈ 12 min, LOD*: 0.2 ng mL ⁻¹ (As), 0.5 ng mL ⁻¹ (Sb), RSD [#] : <2% and 3% (for As and Sb)	28
As, Sb, Se	Water samples	Anion exchange Hamilton PRX-X100 (250 mm × 4.1 mm, 10 μm)	Isocratic elution: 12.5 mM $(\text{NH}_4)_2\text{HPO}_4$ + 3% (v/v) methanol pH = 8.5 (with NH_4OH)	As(III), As(V), MMA, DMA, Sb(V), Se(IV), Se(VI)	Flow = 1.5 mL min ⁻¹ , injection volume = 100 μL, time: ≈ 20 min	17

^a AsC: arsenocholine; TMAO: trimethylarsine oxide; TeMA: tetramethylarsonium ion; MA: methylarsonate; DMA: dimethylarsinate; AsB: arsenobetaine; * limit of detection. [#] relative standard deviation.

Sb(III, V), and Se(IV, VI). The instrumental conditions and tuning information are given in Table 2. The inlet system consisted of a Scott type double pass spray chamber (G.E.) and a Conikal nebulizer (G.E.), whose uptake rate was compatible with the flow rate of the HPLC (1.5 mL min^{-1}). For As and Sb, isotopes of ^{75}As and ^{121}Sb were monitored. For Se, the less abundant isotope of ^{78}Se or ^{82}Se had to be used due to the $^{40}\text{Ar}^{40}\text{Ar}$ interference on ^{80}Se . The medium and high resolution modes of the mass spectrometer were checked. However the medium resolution mode was favored because it provided a higher sensitivity than in high-resolution mode and would not cause interference for As analysis. Optimum sensitivity and signal stability after coupling to the HPLC were achieved by adjusting the nebulizer gas slightly (typical setting of 1.0 L min^{-1}). The signal intensity (based on $10 \mu\text{g L}^{-1}$ standard) for the monitored isotopes are listed in Table 2.

2.1.2 Separation. The high-pressure liquid chromatographic separations were carried out using a Thermo Scientific Accela 1250 Pump and an Hamilton PRP-X100 (Hamilton, Reno, USA) anion exchange column ($250 \text{ mm} \times 4.1 \text{ mm}$, $10 \mu\text{m}$) at a constant flow rate of 1.5 mL min^{-1} . The instrumentation further consisted of a six-port injection valve and a $50 \mu\text{L}$ sample loop. The HPLC column was connected *via* a capillary tube (EzyFit Nebulizer sample Tubing) to a Conikal Nebulizer (G.E.). The chromatography conditions are listed in Table 3. The pHs of all solutions were determined using a pH-meter (pH 340, WTW).

2.2 Reagents and solutions

All solutions were prepared with double deionized water obtained from a Millipore water purification system (MilliQ Advantage A10, $18 \text{ M}\Omega \text{ cm}$).

Table 2 The ICP-MS conditions used in the measurement

Nebulizer	Conikal nebulizer (G.E.)
Nebulizer gas	Around 1.0 L min^{-1}
Spray chamber	Scott type double pass spray chamber (G.E.)
Resolution mode	High resolution (HR), medium resolution (MR)
Monitored isotopes	^{75}As , ^{78}Se (or ^{82}Se), ^{121}Sb
Signal intensity (cps/ $10 \mu\text{g L}^{-1}$)	MR: ^{75}As : 6.0×10^4 ; ^{78}Se : 1.6×10^4 ; ^{121}Sb : 1.2×10^5 HR: ^{75}As : 1.0×10^4 ; ^{78}Se : 3.3×10^3 ; ^{121}Sb : 3.0×10^4

Table 3 The chromatography conditions used during analysis

Column	PRP-X100 ($250 \text{ mm} \times 4.1 \text{ mm}$, $10 \mu\text{m}$) (Hamilton, Reno, USA)
Mobile phase	0–4.5 min: 5 mM EDTA (97%) + methanol (3%) 4.5–5.5 min: linear ramp to 30 mM EDTA (97%) + methanol (3%) 5.5–11 min: 30 mM EDTA (97%) + methanol (3%)
pH	4.7 (adjusted with formic acid)
Flow rate	1.5 mL min^{-1}
Injection volume	$50 \mu\text{L}$
Species	As (III, V), Sb (III, V), and Se (IV, VI)

Stock solutions (1000 mg L^{-1} for each species) were prepared as follows: As(III) from As(III) oxide (As_2O_3 , p.a., ACS, Reag. $\geq 99.0\%$ Sigma-Aldrich) dissolved in 4 g L^{-1} NaOH (ACS, Reag. Merck) and preserved in 2% HCl. As(V) from sodium arsenate dibasic heptahydrate ($\text{Na}_2\text{HAsO}_4 \cdot 7\text{H}_2\text{O}$, ACS reagent, Sigma-Aldrich) dissolved in water. Sb(III) from potassium antimonyl tartrate trihydrate ($\text{C}_8\text{H}_4\text{K}_2\text{O}_{12}\text{Sb}_2 \cdot 3\text{H}_2\text{O}$, ACS, Reag. $\geq 99\%$, Sigma-Aldrich) dissolved in water. Sb(V) from potassium hexahydroxoantimonate ($\text{H}_6\text{KO}_6\text{Sb}$, for the precipitation of sodium, $\geq 99.0\%$, Fluka) dissolved in water. Se(IV) from sodium selenite ($\text{Na}_2\text{O}_3\text{Se}$, 99%, Sigma) dissolved in water. Se(VI) from sodium selenate ($\text{Na}_2\text{O}_4\text{Se}$, p.a., $\geq 98.0\%$, Sigma-Aldrich) dissolved in water. All the stock solutions were kept at $4 \text{ }^\circ\text{C}$ in the dark and analytical standards were prepared daily by appropriate dilution.

The mobile phase was prepared using EDTA (p.a. AppliChem), the pH of which was adjusted with ammonium (Suprapur, Merck) and formic acid (ACS, Reag. 98–100%, Merck). Other acids such as acetic acid (for synthesis, 99–100%, Merck), phosphoric acid (Suprapur, 85%, Merck) and sulfuric acid (GR for analysis, 95–97%, Merck) were also checked. The mobile phase was filtered through a $0.45 \mu\text{m}$ membrane (Whatman) before use. To enhance plasma performance methanol (for HPLC, $\geq 99.9\%$, Sigma-Aldrich) was added to the mobile phase.

SRM 1643e (NIST, National Institute of Standards and Technology) and CRM-SW (High-purity Standards) were used as certified reference materials.

3. Procedure

As a first step As (As(III) and As(V)) and Sb (Sb(III) and Sb(V)) were studied separately under different chromatographic conditions (*e.g.* pH and concentration of mobile phase), with the purpose of exploring information regarding the influence of pH and concentration of the different mobile phases on the retention times. With the knowledge that EDTA works well for the separation of Se,³⁹ EDTA was the eluent of choice. By changing the concentration, flow rate and pH of the EDTA-based mobile phase retention times for As(III), As(V), Sb(III) and Sb(V) were obtained first individually and then later in combination for As(III, V) and Sb(III, V), and eventually As(III, V), Sb(III, V) and Se(IV, VI). The chromatographic conditions were optimized by adjusting the pH slightly with different acids. Phosphoric acid, sulfuric acid, acetic acid and formic acid were tested for the adjustment of pH. To further optimize separation and detection various solvent gradients and different methanol concentrations (*e.g.* 1%, 2% and 3% methanol) were investigated. Those separation and detection conditions deemed most efficient were then validated and tested for stability of retention time, linearity, detection limit and recovery. Finally, the method was applied to the analyses of two hot spring samples from Indonesia labeled as J52 and J54, and two CRMs: SRM 1643e and CRM-SW.

4. Results and discussion

4.1 Development of the speciation analysis method

4.1.1 Speciation of As and Sb. Theoretically, the anions and non-charged molecules of a given elemental species, such as

$\text{H}_3\text{AsO}_3^\circ$ and H_2AsO_4^- , can be separated in an ion exchange column. This is caused by differences in their charges, charge densities and distribution of charge on their surfaces, which results in different degrees of binding with the ion exchanger. These binding abilities can be controlled by varying the chromatographic conditions, particularly ionic strength (*e.g.* concentration of mobile phase) and pH. Speciation of Sb, however, adds additional complexity, because $\text{Sb}(\text{OH})_3^\circ$ normally precipitates in the column. Thus a particular mobile phase is needed in order to stabilize $\text{Sb}(\text{OH})_3^\circ$ in solution. Since Sb has a more complexing chromatographic behavior than As and Se, we chose EDTA as a starting point for the optimization of As and Sb species separation, with the idea that EDTA could chelate $\text{Sb}(\text{III})$ and form a $\text{Sb}(\text{III})$ -EDTA anion. The first step was to investigate retention time as a function of mobile phase concentration. Concentrations of 2 mM, 5 mM, 8 mM, 10 mM and 20 mM were tested on an anion exchange PRP-X100 (250 mm \times 4.1 mm, 10 μm) column. The pH of mobile phase was adjusted to 4.5. The result showed that, the retention times of $\text{As}(\text{III})$ and $\text{Sb}(\text{V})$ more or less remained constant in the concentration range from 2 mM to 20 mM, while on the other hand, the retention times of $\text{As}(\text{V})$ and $\text{Sb}(\text{III})$ decreased, particularly for $\text{Sb}(\text{III})$, whose retention time decreased sharply from 2 mM to 10 mM. Considering the interaction of $\text{Sb}(\text{III})$ and EDTA, it makes sense that the retention time of $\text{Sb}(\text{III})$ was more dependent on the concentration of EDTA. Taking both, resolution and retention time, into consideration, 5 mM seemed to be the optimum concentration of EDTA in the mobile phase, which allowed a relatively short analysis time and good separation of the chromatographic peaks of $\text{As}(\text{V})$ and $\text{Sb}(\text{III})$. For the flow rate of mobile phase, 1.5 mL min^{-1} was favored, as previous work⁴⁰ had shown that 1.5 mL min^{-1} worked well for the $\text{As}(\text{III})$ and $\text{As}(\text{V})$ speciation analysis on an Hamilton PRP-X 100 anion exchange column. A solution containing 10 $\mu\text{g L}^{-1}$ of each $\text{As}(\text{III})$, $\text{As}(\text{V})$, $\text{Sb}(\text{III})$ and $\text{Sb}(\text{V})$ was analyzed with 5 mM EDTA as mobile phase (pH = 4.5). The chromatogram showed that each analyte had a good separation, while the separation as a whole was finished in 16 min.

Our chromatogram revealed an additional peak at around 15 min, which following Hansen *et al.*⁴¹ was interpreted to be that of $\text{Sb}(\text{V})$ -polymer. Since EDTA can not chelate $\text{Sb}(\text{V})$, and thus $\text{Sb}(\text{V})$ -polymer and $\text{Sb}(\text{OH})_6^-$ should elute at different times. Hansen *et al.*⁴¹ assumed that the inability to convert $\text{Sb}(\text{V})$ complexes into one common complex may partly explain the emergence of unidentified peaks in Sb speciation analysis.^{18,22,42} They suggested acidic hydrolysis of samples with 1 M HCl in the presence of chelating ligands such as EDTA and citrate. The same phenomenon was also verified when EDTA and phthalic acid combined were used as mobile phase.⁴³ In this study whenever the unidentified $\text{Sb}(\text{V})$ peak appeared in a chromatogram, it was integrated together with the $\text{Sb}(\text{V})$ peak for the calculations of $\text{Sb}(\text{V})$ linearity and recovery.

4.1.2 Speciation of As, Sb and Se. The chromatographic conditions obtained in the first step were subsequently applied for the separation of $\text{Se}(\text{IV})$ and $\text{Se}(\text{VI})$. However, the result revealed that Se speciation has a strong dependency on the acid used for pH control. Thus different acids, such as phosphoric

acid, sulfuric acid, acetic acid and formic acid were tested for the adjustment of pH of the mobile phase. Eventually phosphoric acid, sulfuric acid and acetic acid were discarded, because they (specially phosphoric acid) led to a surprisingly high baseline and poor peak shape for $\text{Se}(\text{IV})$ and $\text{Se}(\text{VI})$. While we did not investigate this further one could assume that the purity of those acids may have played a role. Once formic acid was chosen as the appropriate acid separation and retention were optimized by adjusting the pH. Because pH can affect the species retention time by changing the existing forms of eluent and solute ions, a solution containing 10 $\mu\text{g L}^{-1}$ of $\text{As}(\text{III})$, $\text{As}(\text{V})$, $\text{Sb}(\text{III})$, $\text{Sb}(\text{V})$ and 100 $\mu\text{g L}^{-1}$ of $\text{Se}(\text{IV})$ and $\text{Se}(\text{VI})$ was analyzed using 5 mM EDTA as a mobile phase in the pH range from 4 to 5. The result revealed that the retention times of $\text{Se}(\text{VI})$ and the unidentified peaks for a $\text{Sb}(\text{V})$ -polymer were shortened by increasing the pH from 4 to 5, while other species remained more or less the same position, indicating less dependence on pH. The behavior of $\text{Se}(\text{VI})$ could be explained solely based on the physicochemical properties of the eluent. EDTA is known for its various protonated forms depending on pH; from $\text{H}_6\text{EDTA}^{2+}$ at very acidic condition to EDTA^{4-} at very basic conditions. It could function as a powerful competing anion and thus has a strong influence on polyvalent anions such as SeO_4^{2-} . The $\text{Sb}(\text{V})$ -polymer was affected greatly by pH, probably due to hydrolysis and change of charged situation of $\text{Sb}(\text{V})$ -polymer in response to the change in pH. Increasing pH shortened of the total analysis time, but at the same time causing deterioration of the $\text{Sb}(\text{III})$ peak shape. Noteworthy, the “unwanted” peak of $\text{Sb}(\text{V})$ -polymer became larger with increasing pH, an observation in accordance with Hansen *et al.*⁴¹ who postulated that the $\text{Sb}(\text{V})$ -polymer peak would become smaller at a lower pH because of acidic hydrolysis. Compromisingly, a pH value of 4.5 was favored as the optimum acidic condition for the mobile phase.

4.2 Optimization of chromatographic conditions

4.2.1 Addition of methanol. Methanol is one of the most commonly used organic compounds for modification of chromatographic conditions, because it can be used to improve signal intensity during ICP-MS detection and changes retention time during speciation analysis.^{17,44} Thus, the logic next step in method development was to investigate the potential to improve separation and detection by adding methanol to the mobile phase. The result was that signal intensity was enhanced greatly for As ($\text{As}(\text{III})$ and $\text{As}(\text{V})$) and Se ($\text{Se}(\text{IV})$ and $\text{Se}(\text{VI})$) when methanol was added to the mobile phase. The intensity for Sb species, however, was only slightly improved. A suggested explanation for this phenomenon is that the loading of carbon-containing polyatomic ions into the plasma leads to a strongly increased population of C^+ and/or carbon-containing polyatomic ions and the degree of ionization of a given analyte is improved by transfer of electrons to the carbon ions (or other carbon-containing ions) from that analyte.⁴⁵ This would indicate that As and Se species were not fully ionized in the plasma. A combination of 3% methanol and 5 mM EDTA provided the optimum chromatographic conditions although it slightly

increased analysis time. To offset this increase the mobile phase pH was changed from 4.5 to 4.7. This shortened the overall analysis time, without remarkable effect on the quality of the peak shapes. The chromatogram obtained under what was considered optimum chromatographic conditions (5 mM EDTA in combination with 3% methanol at pH of 4.7 adjusted with formic acid) showed that all species had a good signal sensitivity and detection was finished in just under 22 min. These species eluted in the order of As(III), Sb(V), As(V), Se(IV), Sb(III) and Se(VI).

4.2.2 Application of a solvent gradient. The first four peaks (As(III), Sb(V), As(V) and Se(IV)) were sufficiently separated and could be eluted in the first 4 min after injection. However, the remaining peaks for Sb(III) and Se(VI) came much later; at 8.3 min for Sb(III) and 19.1 min for Se(VI), indicating that they were strongly retained in the column, which can also be seen from their broad peak shape and long retention time, thus leading to a pretty long overall analysis time of more than 22 minutes. In order to shorten the separation time and to improve the detection limit of Sb(III) and Se(VI), a further modification was made by applying 30 mM EDTA combined with 3% methanol as a solvent gradient which is a common strategy in chromatography.⁴⁶ The gradient program was: 0–4.5 min, 97% 5 mM EDTA and 3% methanol; 4.5–5.5 min, linear ramp to 97% 30 mM EDTA and 3% methanol; 5.5–11 min, 97% 30 mM EDTA and 3% methanol. With this gradient setting the first four peaks were kept in their original position and shape, while the two remaining peaks had improved elution time and peak shape. Thus, the sensitivity of Sb(III) and Se(VI) was improved which ensured a lower detection limit and shortened the overall analysis time to 11 min. Despite the variation in composition of the mobile phase, no shift of the base line was observed, which could be a byproduct of applying a gradient during HPLC separation. A chromatogram of a standard solution containing $0.2 \mu\text{g L}^{-1}$ As(III, V) and Sb(III, V), and $0.5 \mu\text{g L}^{-1}$ Se(IV, VI) is presented in Fig. 1.

4.3 Validation

Following development a complete evaluation was conducted to evaluate stability of retention time, linearity, detection limit and spike recovery of the method.

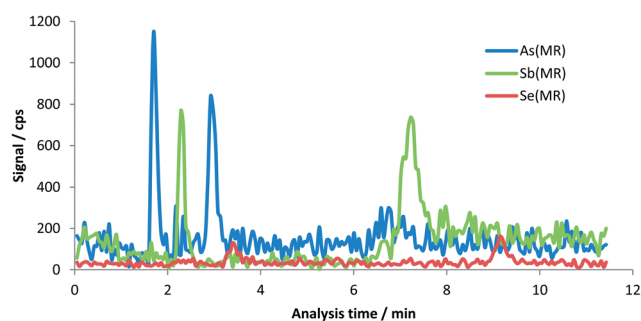


Fig. 1 Chromatogram of a standard containing $0.2 \mu\text{g L}^{-1}$ As(III, V) and Sb(III, V), and $0.5 \mu\text{g L}^{-1}$ Se(IV, VI); The peaks from left to right are As(III), Sb(V), As(V), Se(IV), Sb(III) and Se(VI) respectively.

4.3.1 Stability of retention time. To determine the retention times for the six species replicate measurements were made. The relative standard deviation (RSD) was calculated in order to check its stability (Table 4. Mean \pm RSD, $n \geq 20$). Table 4 shows that the retention times for As(III), As(V), Sb(III), Sb(V), Se(IV) and Se(VI) were 1.70, 2.94, 7.14, 2.28, 3.38 and 9.36 min, respectively. Low RSD of 2% for As(III) and Sb(V) and 4% for As(V) and Se(IV) were obtained from more than 20 replicate measurements. Even after the eluent gradient was introduced, Sb(III) and Se(VI) still had RSDs of less than 10% (8% for Sb(III) and 9% for Se(VI)).

4.3.2 Detection limit. The limit of detection (LOD) was calculated according to the recommendation of the IUPAC (International Union of Pure and Applied Chemistry), as the corresponding concentration of 3 times the standard deviation for the signal/noise (S/N) ratio for each species. Blank solution (Milli-Q water) spiked with concentrations close to the detection limit of all six desired species ($0.2 \mu\text{g L}^{-1}$ for As(III, V) and Sb(III, V), and $0.5 \mu\text{g L}^{-1}$ for Se(IV, VI)) were measured 11 times to calculate the corresponding detection limits. Fig. 1 showed the chromatography close to the detection limit. The detection limits for As(III), As(V), Sb(III), Sb(V), Se(VI) and Se(IV) were $0.02 \mu\text{g L}^{-1}$, $0.06 \mu\text{g L}^{-1}$, $0.2 \mu\text{g L}^{-1}$, $0.02 \mu\text{g L}^{-1}$, $0.2 \mu\text{g L}^{-1}$ and $0.4 \mu\text{g L}^{-1}$ respectively (Table 4), which in general were better than the LODs for those methods listed in Table 1. In addition to S/N , peak height and peak area for each species were also calculated to confirm their detection limits and similar results were obtained.

4.3.3 Linearity. The linearity of each calibration curve was examined for different concentration ranges with at least 5 standard points. The linearity for As(III, V) and Sb(III, V) was investigated for the concentration range from 0.5 to $75 \mu\text{g L}^{-1}$, and the range from 5.0 to $200 \mu\text{g L}^{-1}$ was used for Se(IV, VI), which are the regulatory concentration ranges for many different water types, including ground water.^{47,48} The results showed that detection in these concentrations ranges was linear, as demonstrated by excellent correlation coefficients. The linear correlation coefficients (R^2), obtained from at least 6 replicate experiments, were 0.9999 for As(III) and Se(IV), and 0.9998 for As(V) (Table 4).

4.3.4 Recovery. To our knowledge, only a few methods focused on the simultaneous analysis of As, Se and Sb species in fluid samples have been reported. In the absence of a certified reference material (CRM), which contains As(III, V), Sb(III, V) and Se(IV, VI) the strategy was to carry out spike recovery experiments for each species, which enabled us to perform a quantitative evaluation of the method. The chromatographic recovery for every individual species was estimated by calculating the quantity of the species eluted from the column as a percentage of the amount injected into the column.

Firstly, a synthetic sample prepared with deionized water with low concentrations approximately from 1.0 to $2.5 \mu\text{g L}^{-1}$ for all species were analyzed. A duplicate sample was spiked with $1.0 \mu\text{g L}^{-1}$ As(III, V), Sb(III, V) and $2.0 \mu\text{g L}^{-1}$ Se(IV, VI). Both the synthetic sample and the spiked one were measured 3 times and the spike recovery was calculated (Table 5). Subsequently,

Table 4 The concentration range, correlation coefficient, detection limit and retention times for six species. The correlation coefficients were obtained from at least 6 replicate experiments. The detection limit was calculated from 11 replicate measurements of blank. The retention times were obtained from at least 20 replicate measurements

	Concentration range/ $\mu\text{g L}^{-1}$	Correlation coefficient/ R^2	Limit of detection (LOD)/ $\mu\text{g L}^{-1}$	Retention time/min
As(III)	0.5–75	0.9999	0.02	1.70 \pm 0.02
As(V)	0.5–75	0.9998	0.06	2.94 \pm 0.04
Sb(III)	0.5–75	0.9998	0.2	7.14 \pm 0.08
Sb(V)	0.5–75	0.9998	0.02	2.28 \pm 0.02
Se(IV)	5.0–200	0.9999	0.2	3.38 \pm 0.04
Se(VI)	5.0–200	0.9998	0.4	9.36 \pm 0.09

spike recoveries were tested using two “real” samples labeled as J52 and J54. The two samples were from two hot springs in Cisolok and Patuha on Java Island, Indonesia. The initial temperature and pH for sample J52 in the field were 102.0 °C and 8.1 and the initial temperature and pH for sample J54 were 32.9 °C and 1.0. Both J52 and J54 were chloride rich samples; 305.6 mg L⁻¹ for J52 and 35.2 mg L⁻¹ for J54. The samples were acidified with HCl and preserved in the dark at room temperature after sampling. These two samples were diluted 5 fold with deionized water prior to spiking to bring the concentrations into the calibration and linearity range of the method. For sample J52, 20 $\mu\text{g L}^{-1}$ As(III, V), 1.0 $\mu\text{g L}^{-1}$ Sb(III, V) and 5.0 $\mu\text{g L}^{-1}$ Se(IV, VI) were added as spikes. For sample J54, 5 $\mu\text{g L}^{-1}$ As(III), Se(IV, VI) and 0.5 $\mu\text{g L}^{-1}$ Sb(III, V), As(V) were added. Each sample (with and without spikes) was measured at least 3 times and the results are listed in Table 5. It can be seen that: (i) except the recovery of As(III) for synthetic sample (89%) and Sb(III) for sample J52 (123%), all the other species had a spike recovery of 90–110%, indicating that almost no mass loss happen in chromatography. (ii) In the two analyzed hot spring samples, the concentration of As is much higher than Sb and Se. In

sample J52 only As(V) and Sb(V) were detectable probably because of oxidation caused by inappropriate preservation. (iii) Although, in the two hot spring samples no Se species were determined. However, the good recovery (98.8% and 107.6% for Se(IV), and 97.8% and 109.4% for Se(VI)) indicated that the proposed method could be successfully applied to Se(IV, VI) speciation analysis in real samples.

4.4 Application and matrix interference

The proposed method was finally applied to two CRMs: SRM 1643e (NIST, National Institute of Standards and Technology) and CRM-SW (High-purity Standards). It is worth noting that in the CRM-SW no Sb species were present. The two CRMs were measured without dilution, and 3 replicate measurements were carried out. In SRM 1643e As(V) was predominant and only trace amounts of As(III) were detected. In the case of Sb and Se, only Sb(V) and Se(IV) were detected. In CRM-SW, only As(V) and Se(IV) were detected. The results were in good agreement with the certified values (Table 6).

Matrix interferences were evaluated, including the potential ⁴⁰Ar³⁵Cl⁺ interference on As analysis, and the matrix effect on

Table 6 The results of certified reference materials SRM 1643e and CRM-SW. Data obtained from 3 replicate measurements^a

Sample	Species	Determined ($\mu\text{g L}^{-1}$)	Certified ($\mu\text{g L}^{-1}$)
SRM 1643e	As(III)	0.62 \pm 0.07	60.45 \pm 0.72
	As(V)	58.03 \pm 0.87	
	Sb(III)	ND	
	Sb(V)	58.40 \pm 2.63	
	Se(IV)	11.85 \pm 0.51	
	Se(VI)	ND	
CRM-SW	As(III)	ND	20.00 \pm 0.00
	As(V)	20.80 \pm 1.40	
	Se(IV)	4.42 \pm 0.39	
	Se(VI)	ND	

^a ND: not determined.

Table 5 Spike recovery of a synthetic sample and two hot spring samples J52 and J54. The data was obtained from at least 3 replicate measurements for each sample

	Synthetic sample			Sample J52			Sample J54		
	Spike ($\mu\text{g L}^{-1}$)	Determined ($\mu\text{g L}^{-1}$)	Recovery (%)	Spike ($\mu\text{g L}^{-1}$)	Determined ($\mu\text{g L}^{-1}$)	Recovery (%)	Spike ($\mu\text{g L}^{-1}$)	Determined ($\mu\text{g L}^{-1}$)	Recovery (%)
As(III)	0.0	1.03 \pm 0.02	—	0.0	0	—	0.0	3.89 \pm 0.02	—
	1.0	1.92 \pm 0.01	89.0	20.0	18.83 \pm 0.83	94.2	5	8.59 \pm 0.31	94
As(V)	0.0	1.21 \pm 0.01	—	0	19.45 \pm 0.56	—	0.0	0	—
	1.0	2.11 \pm 0.01	90	20.0	38.83 \pm 0.70	96.9	0.5	0.51 \pm 0.01	102
Sb(III)	0.0	1.58 \pm 0.02	—	0	0	—	0.0	0.40 \pm 0.01	—
	1.0	2.53 \pm 0.03	95	1.0	1.23 \pm 0.09	123	0.5	0.90 \pm 0.00	100
Sb(V)	0.0	1.56 \pm 0.01	—	0	0.83 \pm 0.06	—	0.0	0.38 \pm 0.02	—
	1.0	2.62 \pm 0.07	106	1.0	1.77 \pm 0.11	94	0.5	0.87 \pm 0.01	98
Se(IV)	0.0	2.21 \pm 0.06	—	0	0	—	0.0	0	—
	2.0	4.10 \pm 0.06	94.5	5.0	4.94 \pm 0.59	98.8	5	5.38 \pm 0.04	107.6
Se(VI)	0.0	2.08 \pm 0.01	—	0	0	—	0.0	0	—
	2.0	3.95 \pm 0.06	93.5	5.0	4.89 \pm 0.20	97.8	5	5.47 \pm 0.08	109.4

species retention time and results. In order to check if Cl^- can cause interference for As species, a standard solution containing $10 \mu\text{g L}^{-1}$ of the six desired species and $500 \mu\text{g L}^{-1}$ Cl^- was injected into the column. The result showed that Cl^- was eluted at 6.11 min, indicating that it would not cause any interference for As analysis because As(III) and As(V) were eluted at 1.70 and 2.94 min respectively. The retention times of the six species were evaluated again when analyzing the two hot spring samples and the two CRMs. The results showed no shift for those species detected in the hot spring samples. In SRM 1643e and CRM-SW, the detected species generally showed a slightly earlier elution than the standards. However, no obvious matrix influence could be inferred.

5. Conclusion

In this paper, a new simultaneous speciation analysis method focused on inorganic redox species of As(III, V), Sb(III, V), and Se(IV, VI) based on HPLC-SF-ICP-MS was developed using an anion exchange column. EDTA combined with 3% methanol was used as mobile phase. The total analysis time was less than 11 minutes by introducing in a solvent gradient. The inlet system of detection consisted of a Scott type double pass spray chamber and a conical nebulizer. All species were measured free of interference. Linear correlation coefficients of ≥ 0.9998 for all calibration curves were obtained. The method showed a low detection limit, generally lower than related report, for each desired species. Most species in the analyzed samples had a spike recovery of 90–110%. No inter-conversion between species or mass loss during chromatography was observed. The study confirmed the complexing property of Sb that Sb(III) rather than Sb(V) had a strong affinity in the column, and Sb(V) existed in the form of $\text{Sb}(\text{OH})_6^-$ and Sb(V)-polymer. The method is characterized with simple eluent composition, short overall analysis time, low detection limit, good linearity and reliable repeatability of retention time, and thus could be safely applied to a variety of fluid samples.

Acknowledgements

We thank Maria Jose Ruiz-Chancho for her constructive help at the early age of the study. Also thank Budi Joko Purnomo for his donation of the two hot spring samples collected from Java, Indonesia. TP acknowledges support by the German Research Foundation (DFG).

References

- 1 C. Breuer and T. Pichler, *Chem. Geol.*, 2013, **348**, 2–14.
- 2 Y. N. Vodanyanskii, *Eurasian Soil Sci.*, 2010, **43**, 37–46.
- 3 A.-K. Leuz, *Ph.D. Dissertation*, University of Oldenburg, 2006.
- 4 R. E. Price, J. London, D. Wallschläger, M. J. Ruiz-Chancho and T. Pichler, *Chem. Geol.*, 2013, **348**, 48–55.
- 5 B. J. Mailloux, E. Alexandrova, A. R. Keimowitz, K. Wovkulich, G. A. Freyer, M. Herron, J. F. Stolz, T. C. Kenna, T. Pichler, M. L. Polizzotto, H. Dong, M. Bishop and P. S. K. Knappett, *Appl. Environ. Microbiol.*, 2009, **75**, 2558–2565.
- 6 R. E. Price, J. P. Amend and T. Pichler, *Appl. Geochem.*, 2007, **22**, 2595–2605.
- 7 V. Jamier, L. A. Ba and C. Jacob, *Chem.-Eur. J.*, 2010, **16**, 10920–10928.
- 8 Y. Nakamaru and K. Sekine, *Soil Sci. Plant Nutr.*, 2008, **54**, 332–341.
- 9 K. M. Campbell, D. Malasarn, C. W. Saltikov, D. K. Newman and J. G. Hering, *Environ. Sci. Technol.*, 2006, **40**, 5950–5955.
- 10 S. C. Wilson, P. V. Lockwood, P. M. Ashley and M. Tighe, *Environ. Pollut.*, 2010, **158**, 1169–1181.
- 11 Y. Li, B. Hu, M. He and G. Xiang, *Water Res.*, 2008, **42**, 1195–1203.
- 12 M. Moldovan, E. M. Krupp, A. E. Holliday and O. F. X. Donard, *J. Anal. At. Spectrom.*, 2004, **19**, 815–822.
- 13 J. Zheng, H. Hintelmann, B. Dimock and M. S. Dzurko, *Anal. Bioanal. Chem.*, 2003, **377**, 14–24.
- 14 J. A. Day, M. Montes-Bayón, A. P. Vonderheide and J. A. Caruso, *Anal. Bioanal. Chem.*, 2002, **373**, 664–668.
- 15 L. S. Milstein, A. Essader, E. D. Pellizzari, R. a. Fernando and O. Akinbo, *Environ. Int.*, 2002, **28**, 277–283.
- 16 A. J. Bednar, J. R. Garbarino, M. R. Burkhardt, J. F. Ranville and T. R. Wildeman, *Water Res.*, 2004, **38**, 355–364.
- 17 T. Guerin, M. Astruc, A. Batel and M. Borsier, *Talanta*, 1997, **44**, 2201–2208.
- 18 N. Miekeley, S. R. Mortari and A. O. Schubach, *Anal. Bioanal. Chem.*, 2002, **372**, 495–502.
- 19 S. Canepari, E. Marconi, M. L. Astolfi and C. Perrino, *Anal. Bioanal. Chem.*, 2010, **397**, 2533–2542.
- 20 M. Krachler, H. Emons and J. Zheng, *Trends Anal. Chem.*, 2001, **20**, 79–90.
- 21 P. Smichowski, Y. Madrid and C. Cámara, *Fresenius' J. Anal. Chem.*, 1998, **360**, 623–629.
- 22 H. R. Hansen and S. A. Pergantis, *Anal. Chem.*, 2007, **79**, 5304–5311.
- 23 J. Zheng, A. Iijima and N. Furuta, *J. Anal. At. Spectrom.*, 2001, **16**, 812–818.
- 24 G. Ceriotti and D. Amarasiriwardena, *Microchem. J.*, 2009, **91**, 85–93.
- 25 K. Takayanagi and D. Cossa, *Water Res.*, 1997, **31**, 671–674.
- 26 T. Lindemann, A. Prange, W. Dannecker and B. Neidhart, *Fresenius' J. Anal. Chem.*, 1999, **364**, 462–466.
- 27 L. Orero Iserte, A. F. Roig-Navarro and F. Hernández, *Anal. Chim. Acta*, 2004, **527**, 97–104.
- 28 Y. Morita, T. Kobayashi, T. Kuroiwa and T. Narukawa, *Talanta*, 2007, **73**, 81–86.
- 29 P. C. Uden, *Anal. Bioanal. Chem.*, 2002, **373**, 422–431.
- 30 X. Dauchy, M. Potin-Gautier, A. Astruc and M. Astruc, *Fresenius' J. Anal. Chem.*, 1994, **348**, 792–805.
- 31 C. B'Hymer and J. A. Caruso, *J. Chromatogr. A*, 2006, **1114**, 1–20.
- 32 J. Bowman, B. Fairman and T. Catterick, *J. Anal. At. Spectrom.*, 1997, **12**, 313–316.
- 33 J. Y. Cabon and C. Louis Madec, *Anal. Chim. Acta*, 2004, **504**, 209–215.

- 34 H. Wu, X. Wang, B. Liu, Y. Liu, S. Li, J. Lu, J. Tian, W. Zhao and Z. Yang, *Spectrochim. Acta, Part B*, 2011, **66**, 74–80.
- 35 B. A. Fernandez, C. V. Temprano, M. R. F. Campa, A. Sanz-Medel and P. Neil, *Talanta*, 1992, **39**, 1517–1523.
- 36 I. Ipolyi and P. Fodor, *Anal. Chim. Acta*, 2000, **413**, 13–23.
- 37 L. Kozak and P. Niedzielski, *Anal. Lett.*, 2011, **44**, 2312–2320.
- 38 R. C. Richter, K. Swami, S. Chace and L. Husain, *Fresenius' J. Anal. Chem.*, 1998, **361**, 168–173.
- 39 B. R. E. Wolf, S. A. Morman, J. M. Morrison and P. J. Lamothe, *Simultaneous Speciation of Arsenic, Selenium, and Chromium by HPLC-ICP-MS*, Denver, 2008.
- 40 M. J. Ruiz-Chancho, T. Pichler and R. E. Price, *Chem. Geol.*, 2013, **348**, 56–64.
- 41 C. Hansen, B. Schmidt, E. H. Larsen, B. Gammelgaard, S. Stürup and H. R. Hansen, *Analyst*, 2011, **136**, 996–1002.
- 42 S. Foster, W. Maher, F. Krikowa, K. Telford and M. Ellwood, *J. Environ. Monit.*, 2005, **7**, 1214–1219.
- 43 S. Amereih, T. Meisel, E. Kahr and W. Wegscheider, *Anal. Bioanal. Chem.*, 2005, **383**, 1052–1059.
- 44 N. Ulrich, *Anal. Chim. Acta*, 1998, **359**, 245–253.
- 45 E. H. Larsen and S. Stürup, *J. Anal. At. Spectrom.*, 1994, **9**, 1099–1105.
- 46 K. Müller, B. Daus, J. Mattusch, H.-J. Stärk and R. Wennrich, *Talanta*, 2009, **78**, 820–826.
- 47 J. A. Plant, D. G. Kinniburgh, P. L. Smedley, F. M. Fordyce, B. A. Klinck and B. G. Survey, *Treatise Geochem.*, 2006, **9**, 17–66.
- 48 M. Filella, N. Belzile and Y. Chen, *Earth-Sci. Rev.*, 2002, **59**, 265–285.